

# TECHNOMAC

MEDICAL SYSTEMS PVT. LTD.



## COMPANY PROFILE

### ● Present Business Activity Of The Company

M/s TECHNOMAC was established in April 2000. The company began its full scale operation in April, 2002. The company presently works as a manufacturer of X-ray dental machine in normal analog to RVG compatible which meets the latest technologies in dental field.

### ● Directors/Promoters

The promoters as well director Mr. Dhiraj Kumar Sharma have more than 25 years of experience in dental equipment with specialization in X-ray machine. The company keep on growing under his supervision. Also, he leads day to day research and developed of new model of X-ray machine to fulfill the requirement of new technologies to help doctors work with greater efficiency.

### ● Staff

The company has skilled staff of 10, those activate all decision of the senior person in sourcing and manufacturing.

### ● Accounts

Accounts department provides all MIS report to the director and help him to make future plan more conveniently, which help them to grow their business without any resistance.

### ● Turnover

In the last financial year the company achieved Rs. 40 Lakhs in the immediate preceding year 2018-2019. In the current financial year we are on the way to achieve our target.

## Journey Of A Thousand Miles Begin With A Single Step.

### ● Vision

Manufacture advance technology based machinery towards innovative approach.

### ● Mission

The mission of TECHNOMAC to provide high quality machines at best prices.

### ● For How Long

We are manufacturing since 1992.

Till now we are in market with the renowned name TECHNOMAC.


We are practicing every day to introduce quality-oriented machines.

persons from marketing, retailers, buyers, hospitals and clinics are most welcome.

### ● Our Commitment

We are committed to provide quality assurance with services.

# We Are Into Country / State

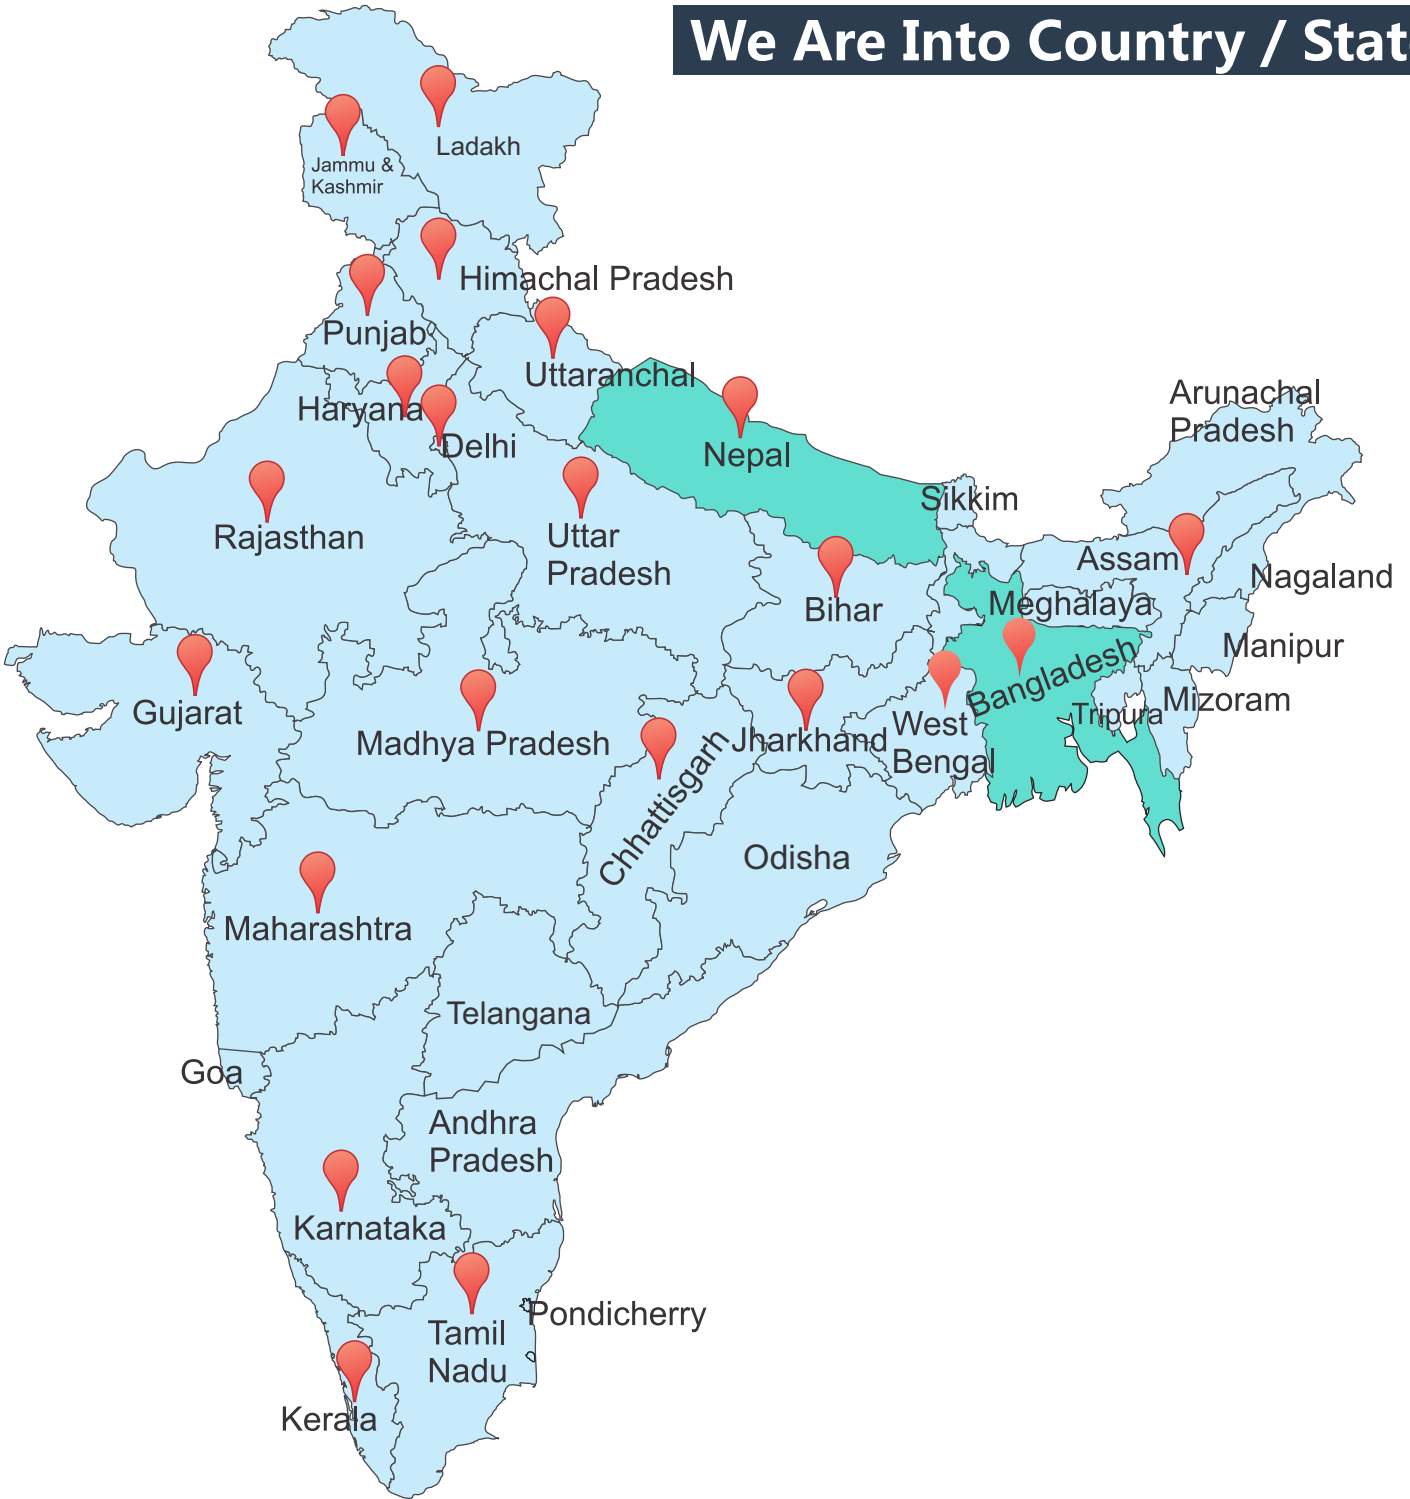

IS 7620 PART-1



CM/L-8100110785

**SALENT FEATURES**

- All Directional movement with angular indication enabling perfect positioning.
- Last exposure selection retained in memory.
- Exposure with remote as well from timer.
- Time delay of 10 sec. between two consecutive exposures.
- Lead coated radiography long cone.
- RVG Mode for digital imaging.
- Soft touch timing selection.
- In-Built stablizer.
- Digital display.

**TECHNICAL SPECIFICATION**

X-Ray Output	: 60Kv, 10mA
Tube Filtration	: 1.5mm Al
Focal point	: 0.8mm
Focus skin distance	: 20cm
Safety leakage radiation	: <30mR/h at 1m distance
Time Range (Digital)	: 0.01 sec. - 3.0 sec
Line voltage	: 190V to 260V
Compensation	
Power supply	: 230V, 50Hz, 5A



MR-01/60 Scissor Arm Wall Model



MR-01/60 Wall Model



MR-01/60 Scissor Arm Floor Model



MR-01/60 Floor Model



Hospitals	College	Trust Societies
Max Fort	Manav Rachna Dental College	Bangla Sahib Trust Society
Apollo	Sharda University	Arya Samaj Trust Society
Fortis	Bankey Bihari Dental College	Maharishi Charak Charitable
Paras	Eklavya Dental College	
E.S.I.	JCD Dental College	
Lady Willingdon		
Saroj Hospital		

Hospitals, Clinics

Colleges

Trust Societies

We are register with :-

1. Aditi (Society)
2. IDA
3. Famdent



**भारत सरकार**  
GOVERNMENT OF INDIA  
**एटॉमिक एनर्जी रेग्युलटरी बोर्ड**  
ATOMIC ENERGY REGULATORY BOARD

Case File Number: 2017-181-V02-001  
Document Number: 15A-362507  
Issuance Date: 12/02/2019  
Expiry Date: 12/02/2022

**TYPE APPROVAL FOR DENTAL (INTRA ORAL) EQUIPMENT MODEL MR 01 MANUFACTURED BY TECHNOMAC, INDIA**

In exercise of the powers conferred on Section 14 of the Atomic Energy Act, 1952 read in conjunction with Rule 3 of the Atomic Energy (Radiation Protection) Rules, 2012, the Atomic Energy Regulatory Board (AERB) hereby grants Type Approval to following medical diagnostic x-ray equipment from radiological safety view point:

Type of Equipment	Dental (Intra Oral)
Model Name	MR 01
Name of Manufacturer	TECHNOMAC, India
No. of X-ray tubes	1
Maximum operating voltage	10.000kVp
Maximum operating current	0.000 mA

**TERMS AND CONDITIONS**

- These Terms and Conditions to be read in conjunction with Terms and Conditions of Supplier's Authorization. A copy of this Type Approval and Supplier's Authorization shall be provided to the prospective user.
- The Type Approval becomes invalid if any change is made in the design of above model.
- The Type Approval shall be applied only by Supplier Authorized by AERB and to the user who has obtained requisite permission from AERB to possess the equipment.
- Supplier shall provide 24x7x365 technical assistance team with Quality Assurance team based to utility after installation and commissioning of x-ray equipment and shall be liable to utility.
- The receipt of above mentioned copy of this Type Approval is conditional upon its revocation.

MR. SHYRRA ZHAFRA KHAN  
TECHNOMAC  
GZ-1, 15, SEWAPUR EXTN,UTTAMNAGAR, NEW DELHI, DELHI-110059  
(Competent Authority)

**Certificate of Registration**

This is to certify that  
**The Quality Management System of  
TECHNOMAC**  
RZ-4115, BINDA PUR EXTENSION, UTTAM NAGAR,  
NEW DELHI-110059, INDIA

has been assessed and found to be in accordance with the  
requirements of the management system standard

**ISO 9001:2015**  
for the following scope :

MANUFACTURING OF DENTAL X-RAY MACHINES

CERTIFICATE No. : 10AAG10410

ISSUANCE DATE : 10/11/2018      10 MONTHS validity      11/10/2020  
RENEWAL DATE : 11/11/2022      2nd SURVEILLANCE      11/10/2021

UAF IS FULL MEMBER OF IAF

UKAS MANAGEMENT SYSTEMS INTERNATIONAL

For BSI Certification Assessment Details Please Visit: [www.bsi.com](http://www.bsi.com)

**Otabu**  
Certificate of Compliance

We hereby declare that the individual lot of product complies with the requirements of BS EN 60601-2-13:2014 Medical Diagnostics

**Manufacturer**  
Name : TECHNOMAC  
Address : SE-4, 115, Hindpuri Gate, Uttam Nagar,  
New Delhi, 110059, India  
Product : Dental X-Ray Machine, RVS and MR-01

The Certificate has been performed on basis of the above product quality system covering the design, development and final inspection of the certified product. The validity covers the product, design and type of components as mentioned in the certificate.

**This certificate is based under the following conditions:**

- It applies only to the specific system mentioned in the certificate of compliance.
- Quality management system shall be implemented and maintained as per the certificate.
- The certificate remains valid only if the manufacturing conditions in the certificate are maintained.
- The manufacturer shall be liable for product recall or withdrawal within the certificate.
- The certificate shall be valid only if the manufacturer maintains the quality management system as per the certificate.
- The certificate shall be valid only if the manufacturer maintains the quality management system as per the certificate.
- The certificate shall be valid only if the manufacturer maintains the quality management system as per the certificate.

Date of Registration : 22 January 2019  
1st Surveillance Date : 21 January 2020  
2nd Surveillance Date : 21 January 2021  
Recertification Date (unless the customer renounces) : 21 January 2022

Certificate No: 4188  
Validity of this certificate can be verified at [www.otabucert.com](http://www.otabucert.com)

**Otabu Certification Limited (UK)**  
Validity of this Certificate is subject to Annual Surveillance audits done successfully.  
\*Otabu Certification Limited is a UK Registered company and is a member of the British Standards Institution (BSI).

Suite 45, 88-90 Hatton Garden, London, EC1N 8PN, UK

**PLEASE CALL**

**For Services**

**9711151755**

**For Sales**

**9268825571**

**Office**

**011-45241014**

 [www.dentalxraymachine.com](http://www.dentalxraymachine.com)

 [technomacdental61@gmail.com](mailto:technomacdental61@gmail.com)

 Plot No. 88, Pocket-L, Sector-1, Bawana

Industrial Area, DSIIDC Sub-city, New Delhi-110039

