

TECHNOMAC

MEDICAL SYSTEMS PVT. LTD.



COMPANY PROFILE

● Present Business Activity Of The Company

M/s TECHNOMAC was established in April 2000. The company began its full scale operation in April, 2002. The company presently works as a manufacturer of X-ray dental machine in normal analog to RVG compatible which meets the latest technologies in dental field.

● Directors/Promoters

The promoters as well director Mr. Dhiraj Kumar Sharma have more than 25 years of experience in dental equipment with specialization in X-ray machine. The company keep on growing under his supervision. Also, he leads day to day research and developed of new model of X-ray machine to fulfill the requirement of new technologies to help doctors work with greater efficiency.

● Staff

The company has skilled staff of 10, those activate all decision of the senior person in sourcing and manufacturing.

● Accounts

Accounts department provides all MIS report to the director and help him to make future plan more conveniently, which help them to grow their business without any resistance.

● Turnover

In the last financial year the company achieved Rs. 40 Lakhs in the immediate preceding year 2018-2019. In the current financial year we are on the way to achieve our target.

Journey Of A Thousand Miles Begin With A Single Step.

● Vision

Manufacture advance technology based machinery towards innovative approach.

● Mission

The mission of TECHNOMAC to provide high quality machines at best prices.

● For How Long

We are manufacturing since 1992.

Till now we are in market with the renowned name TECHNOMAC.


We are practicing every day to introduce quality-oriented machines.

persons from marketing, retailers, buyers, hospitals and clinics are most welcome.

● Our Commitment

We are committed to provide quality assurance with services.

We Are Into Country / State

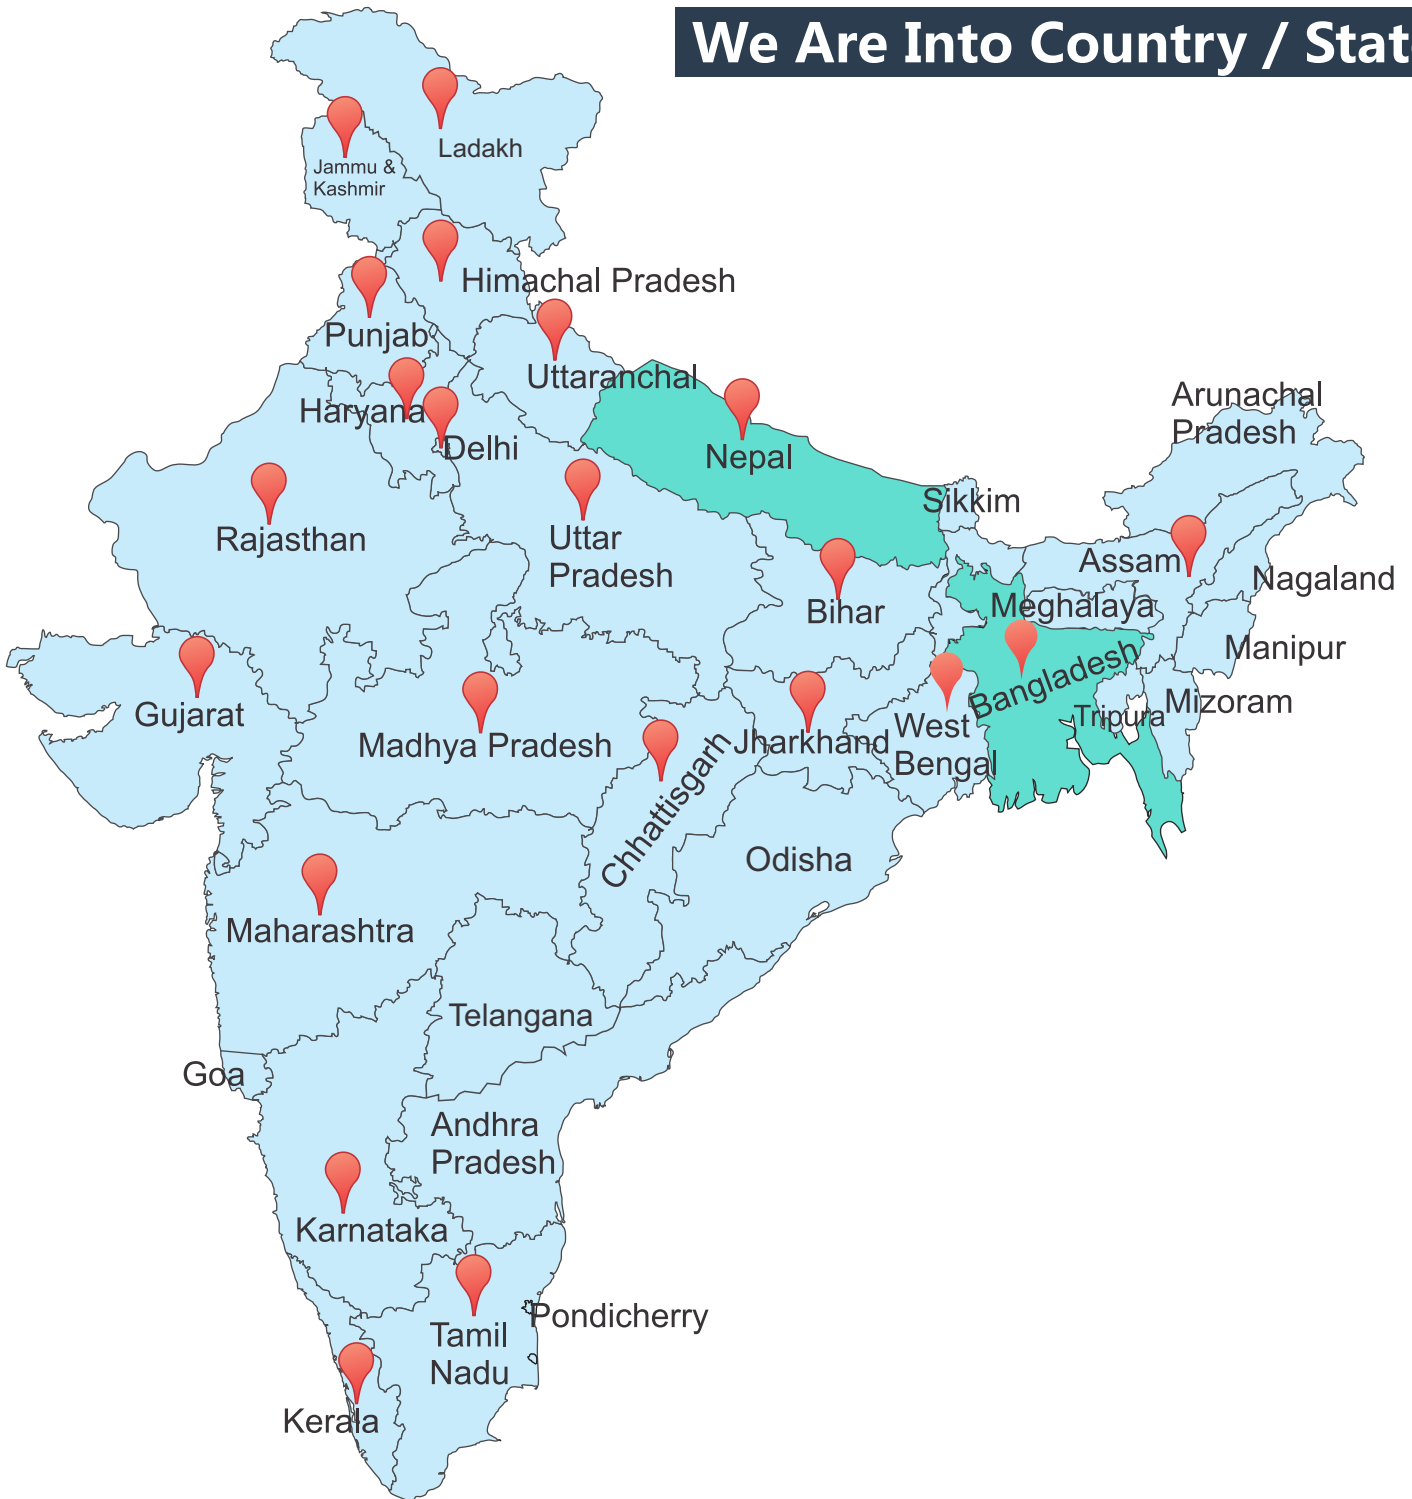

IS 7620 PART-1



CM/L-8100110785

SALENT FEATURES

- All Directional movement with angular indication enabling perfect positioning.
- Last exposure selection retained in memory.
- Exposure with remote as well from timer.
- Time delay of 10 sec. between two consecutive exposures.
- Lead coated radiography long cone.
- RVG Mode for digital imaging.
- Soft touch timing selection.
- In-Built stablizer.
- Digital display.

TECHNICAL SPECIFICATION

X-Ray Output	: 70Kv, 8mA
Tube Filtration	: 1.5mm Al
Focal point	: 0.8mm
Focus skin distance	: 20cm
Safety leakage radiation	: <30mR/h at 1m distance
Time Range (Digital)	: 0.01 sec. - 3.0 sec
Line voltage	: 190V to 260V
Compensation	
Power supply	: 230V, 50Hz, 5A



MR-01 Scissor Arm
Wall Model



MR-01 Wall
Model



MR-01 Scissor Arm
Floor Model



MR-01
Floor Model



Hospitals	College	Trust Societies
Max Fort	Manav Rachna Dental College	Bangla Sahib Trust Society
Apollo	Sharda University	Arya Samaj Trust Society
Fortis	Bankey Bihari Dental College	Maharishi Charak Charitable
Paras	Eklavya Dental College	
E.S.I.	JCD Dental College	
Lady Willingdon		
Saroj Hospital		

Hospitals, Clinics

Colleges

Trust Societies

We are register with :-

1. Aditi (Society)
2. IDA
3. Famdent

PLEASE CALL

For Services

9711151755

For Sales

9268825571

Office

011-45241014

 www.dentalxraymachine.com

 technomacdental61@gmail.com

 Plot No. 88, Pocket-L, Sector-1, Bawana

Industrial Area, DSIIDC Sub-city, New Delhi-110039

